

Spatial In-Body Channel Characterization Using an Accurate UWB Phantom

Carlos Andreu, Sergio Castelló-Palacios, Concepcion Garcia-Pardo, Alejandro Fornes-Leal,
Ana Vallés-Lluch and Narcís Cardona

Abstract— UWB systems have emerged as a possible solution for future wireless in-body communications. However, in-body channel characterization is complex. Animal experimentation is usually restricted. Furthermore, software simulations can be expensive and imply a high computational cost. Synthetic chemical solutions, known as phantoms, can be used to solve this issue. However, achieving a reliable UWB phantom can be challenging since UWB systems use a large bandwidth and the relative permittivity of human tissues are frequency-dependent. In this work, a measurement campaign within 3.1-8.5 GHz by using a new UWB phantom is performed. Currently, this phantom achieves the best known approximation to the permittivity of human muscle in the whole UWB band. Measurements were performed in different spatial positions, in order to investigate also the diversity of the in-body channel in the spatial domain. Two experimental in-body to in-body (IB2IB) and in-body to on-body (IB2OB) scenarios are considered. From the measurements, new path loss models are obtained. Besides, the correlation in transmission and reception is computed for both scenarios. Our results show a highly uncorrelated channel in transmission for IB2IB scenario at all locations. Nevertheless, for IB2OB scenario the correlation varies depending on the position of the receiver and transmitter.

Index Terms— *Body area network, in-body communications, path loss, Ultra-Wideband (UWB) phantom, uncorrelated channel.*

I. INTRODUCTION

Wireless Body Area Networks (WBANs) allow the interconnection between independent nodes located either inside or over the body skin or further. Regarding in-body communications, establishing a proper link with a capsule endoscope [1] or with a pacemaker [2] are examples of technological advances achieved in the last decades. In spite of these healthcare developments, current standards for these kind of communications do not allow high data rate wireless connections, which are common in the current telecommunication services [3]. IEEE Std. 802.15.6 normalized the frequency bands for each propagation scenario.

Concretely, the Medical Implant Communication Service (MICS) band was chosen to enable communication between in-body devices. MICS frequency band (402-405 MHz) has relatively good wave propagation conditions through biological tissues [4]. Nevertheless, this band is constrained to the use of narrow band systems. Particularly, the Industrial, Scientific and Medical (ISM) radio band (2400-2483.5 MHz) has been considered as a candidate in order to enhance the in-body communications in next generation devices [5]. However, these multipurpose bands are widely used for WLAN and WPAN networks so that interferences between services could be produced. Thus, Ultra-Wideband (UWB) frequency range has emerged as a future potential candidate for in-body communications [6]. UWB frequency spectrum covers from 3.1 to 10.6 GHz and its main benefits are high data rate, low power consumption and the low-cost of its transceivers [7]. Nevertheless, the main drawback of UWB for in-body applications is the high attenuation of human body tissues which increases dramatically with the increment of frequency [8]. Hence, an accurate UWB in-body channel characterization is relevant in order to establish a proper link between future UWB implantable nodes.

Implanting devices into human subjects in order to carry propagation measurements out, is not possible due to ethical and physical reasons. Then, some research works have performed in-vivo measurements using living animals such as pigs [9]–[11]. However, the high-cost of each surgical procedure as well as the restrictions in animal experimentations due to ethical reasons are enough arguments to seek other solutions. In the literature, studies based on simulation measurements using human voxel models can be found [12]. Nevertheless, software simulations are not able to reproduce all the channel conditions. Besides, such software simulations can be an expensive solution as well as imply a high complex computational cost. On the other hand, chemical solutions, which emulate the electromagnetic behavior of human body tissues (i.e., complex relative permittivity), have been used in order to recreate the propagation through human tissues [5]. These mimicking materials are known as “phantoms” and have been used in previous propagation studies [13]. Nevertheless, the results obtained with these phantoms are far from the results obtained with living tissues [10]. Even though there are many phantoms that can reproduce the propagation medium with a relative accuracy within narrow frequency bands, only a few are provided for wide frequency bands. An aqueous solution of sugar has been

This work was supported by the Ministerio de Economía y Competitividad, Spain (TEC2014-60258-C2-1-R, TEC2014-56469-REDT), by the European FEDER funds.

C. Andreu, C. Garcia-Pardo, A. Fornes-Leal, and N. Cardona are with the iTEAM, Universitat Politècnica de València, 46022 Valencia, Spain (e-mail: caranes@iteam.upv.es; cgpardo@iteam.upv.es; alforlea@iteam.upv.es; ncardona@iteam.upv.es).

S. Castelló-Palacios and A. Vallés-Lluch are with the Centre for Biomaterials and Tissue Engineering, Universitat Politècnica de València, 46022 Valencia, Spain (e-mail: sercaspa@etsii.upv.es; avalles@ter.upv.es).

reported as UWB phantom [14], but its behavior is far from the real values reported in [8]. Other attempts have been made for wide-band phantoms, but their accuracy decreases as frequency increases [15]. In particular, the reported phantoms of muscle for wide bands show a quite bad approximation above 4-5 GHz [16], mainly regarding the conductivity part.

UWB frequency band aims at enhancing the current in-body applications. In order to improve the UWB channel performance, channel diversity of these systems can be exploited. For instance, current UWB systems have achieved accurate localization techniques [17]. These techniques benefit, among other features, from the diversity of the channel. These localization techniques can be influenced due to the correlation between receivers [18]. In literature, many research works devoted to study the diversity performance of off-body systems can be found [19]. However, to the best of the authors' knowledge not many studies about the UWB in-body channel diversity considering experimental scenarios are addressed in literature.

This work aims at contributing to the UWB in-body channel characterization within 3.1-8.5 GHz by using a new realistic UWB phantom which emulates the electromagnetic behavior of human muscle, as described in [8], with high accuracy in the whole frequency band considered [20]. Two in-body scenarios are considered depending on the location of the receiving antenna: in-body to in-body (IB2IB) and in-body to on-body (IB2OB) scenarios. Besides, a large amount of measurements has been provided by means of a novel spatial experimental setup using a three-dimensional automatic positioner. Hence, the path loss for both IB2IB and IB2OB can be characterized with high accuracy. Moreover, the correlation in transmission and reception is assessed from the measurements. For correlation in transmission, the channel impulse responses between different transmitting antenna positions are considered for a fixed position of the receiving antenna. The correlation at the receiving side is computed in an analogous form.

The remainder of this work is organized as follows: In section II, the measurement setups as well as the methodology are detailed. In section III, the experimental path loss models for each scenario are presented. Section IV shows the correlation in transmission and reception for each scenario. Finally, section V summarizes the conclusions obtained from this work.

II. MEASUREMENT SETUP & METHODOLOGY

A. Experimental scenarios

Regarding the location of the antennas, two different scenarios were emulated:


- In-Body to In-Body (IB2IB), where both antennas are considered to be located inside the human body.
- In-Body to On-Body (IB2OB), where the in-body antenna is considered to be located inside the body whereas the on-body antenna is placed over the human body surface.

B. UWB Phantom


Since the operation environment of these antennas is supposed to be the human body, in which it is not possible to test them, it becomes necessary to employ a tissue-equivalent medium. In this case, as muscle is the main human tissue or at least the future propagation medium for most wireless applications, a muscle-mimicking phantom was considered for our experiments. Keeping in mind that the antennas must be introduced and moved inside the phantom due to our scenarios, the required phantom should be liquid. For this purpose, the phantom proposed here is an aqueous solution of 54.98% acetonitrile and 1.07% NaCl which owns the targeted conditions [20] and is easily prepared as follows: firstly, salt and acetonitrile were poured into a beaker in their corresponding amount, then the required mass was filled with water and stirred for ten minutes until dissolution. This phantom was designed at 24 degrees Celsius. At such temperature, our solution reproduces the dielectric values of human muscle that were characterized at body temperature as reported in [8]. The variation of its dielectric properties with temperature is about ± 0.08 units per degree Celsius for the dielectric constant, and ± 0.11 units per degree for the loss factor. The key of this phantom is the use of acetonitrile, a polar molecule that gets dielectric constant values similar to those of muscle within a wide frequency band. Moreover, the addition of salt increases the loss factor so the tissue's behavior is better imitated in both parts of the complex relative permittivity:

$$\epsilon_r = \epsilon_r' - j\epsilon_r'', \quad (1)$$

where ϵ_r' is the dielectric constant and ϵ_r'' is the loss factor. In Fig. 1, the complex relative permittivity of our muscle phantom is compared to the reported measured values for real muscle tissue [8].

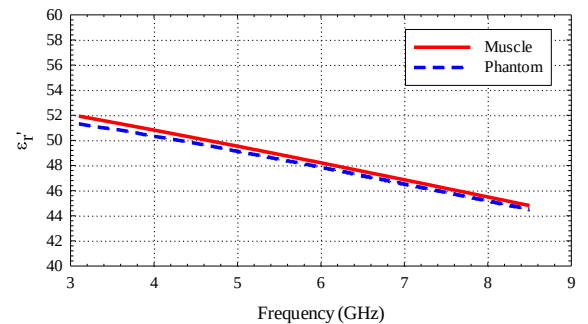

(a) Dielectric constant.

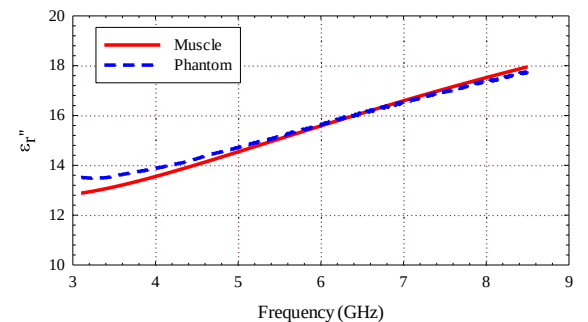

(b) Loss Factor.

Fig. 1. Measured relative permittivity of the UWB phantom compared to the values of human muscle tissue reported in [8].

This phantom is, to the best of the authors' knowledge, the most accurate imitation for the human muscle within the UWB frequency band. In fact, it is worth mentioning that the maximum relative deviation from phantom values compared to real tissue is 1.2% for the real part and 4.85% for the imaginary one, which occurs at 3 GHz.

C. Antennas

In order to perform a reliable UWB in-body measurement campaign, the antennas play a crucial role. They should have a compact structure in order to be implanted inside the human body in different locations as well as to be located over the body surface. Regarding implanted transmitter, an antenna matching within the whole UWB frequency band is essential. Besides, an omnidirectional radiation pattern to communicate with a sensor array located around or inside the body should be achieved. In Fig. 2, the two UWB monopole antennas used in the measurement campaign are depicted. One antenna is approximately 2.2 times larger than the other. The small antenna, which is located at the center of Fig. 2, is an UWB monopole with microstrip feeding. The overall size is 23x20 mm². This miniaturized antenna was designed taking into account the human muscle permittivity values described in [8]. Thus, antenna matching as well as a quasi-omnidirectional radiation pattern in XZ-plane within the UWB frequency range was achieved. Hereinafter, this antenna will be referred to as miniaturized antenna.



Fig. 2. UWB monopoles antennas used in both experimental scenarios.

The large antenna also presents a quasi-omnidirectional radiation pattern in the XZ-plane in the UWB frequency band. Further details of this antenna are given in [21]. Hereinafter, we refer to this antenna as large antenna. This antenna can be used as implanted transmitting antenna as well as on-body or off-body receiver [10]. Besides, both in-vivo and phantom-based measurement campaigns using the large antenna were performed [10], [22].

For the two scenarios previously described, the miniaturized antenna acted as the transmitting antenna, whereas the large antenna was the receiving one. Thus, the large antenna was fixed inside the phantom as in-body antenna for the IB2IB case and outside the liquid phantom as on-body antenna for the IB2OB scenario.

D. Measurement Setup

During measurements, the forward transmission coefficient (S_{21}) was measured and processed for both scenarios. To perform this task, the antennas were connected to a vector network analyzer (hereafter referred to as VNA) which works up to 8.5 GHz. For both scenarios, the antennas were connected to port 1 and 2 of the VNA by means of 2-meter length cables. In order to suppress the effect of the cables and connectors, the VNA was calibrated through a *thru*-calibration. The return loss of the antennas was measured

previously in each measurement point in order to ensure antenna matching across the whole frequency band.

The output power of the VNA was set to 8 dBm with a resolution bandwidth of $f_{\text{IF}} = 3$ kHz. Measurements were performed from 3.1 to 8.5 GHz with $N = 1601$ resolution points resulting in a resolution frequency of $\Delta f = 1.875$ MHz. Five snapshots of the channel were taken in order to enhance the signal-to-noise ratio (SNR). The noise floor was different for each scenario, due to the change in antenna parameters of the receiving antenna. Thus, the noise level in the IB2IB and IB2OB scenarios was at -95 dBm and -88 dBm, respectively.

The new UWB liquid phantom was poured into a Polypropylene (PP) container. The container dimensions were 30x30x15 cm³ with negligible wall thickness. The overall size of the box was chosen in order to mimic a cross section of the human torso. The dimensions in XY-plane are widely used in simulation setups using voxel models [23]. Before being submerged into the UWB phantom, the antenna was covered with a layer of latex so that physical contact between antennas and liquid phantom was avoided. Latex rubber is widely used in healthcare environments. The antenna was carefully wrapped in order to remove the air as well as achieve an air-tight seal.

With the aim of performing channel measurements for different spatial positions, the miniaturized antenna was mounted in a robotic arm and moved to several (x,y,z) locations inside the liquid phantom by using a 3-axis positioner. The error of this positioner is lower than 0.254 mm per cm in each axis. In order to avoid disturbance during measurement time, the access to the room was restricted for everyone. Besides, possible interfering devices were switched off and the surrounding elements were at a minimum distance of 2 meter far from the measurement setup. A fixed temperature of 24°C during the measurements in both setups was assured by means of a thermostat located in the measurement room.

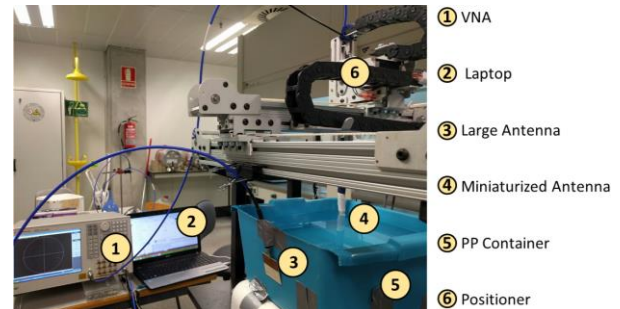


Fig. 3. Experimental measurement setup particularized for IB2OB scenario.

The miniaturized antenna was moved in steps of $\Delta x = \Delta y = \Delta z = 1$ cm along X, Y and Z axes, respectively. Considering the step resolution as well as the distance between each antenna and the internal container's walls, the distance between the antenna centers, d , can be computed. During measurements, the positioner stopped in each location until the VNA had finished the acquisition. In order to control and synchronize the positioner and the VNA to perform the measurements, a software was designed in Visual Studio.

Fig. 4 depicts the measurement setup particularized for the IB2IB scenario. The large antenna was placed in the middle of the Y axis, at 8 cm away from the container's wall located

behind it (X axis), and at a height of 8.6 cm from the container's floor (Z axis). The miniaturized antenna was located in a XYZ mesh of $11 \times 11 \times 2$ measurement points.

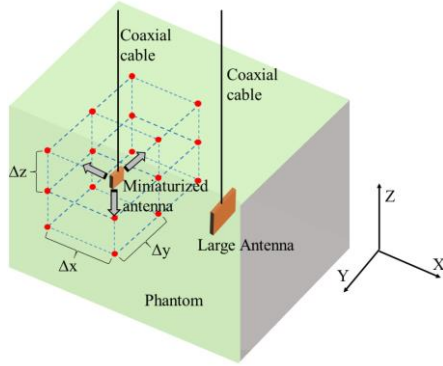


Fig. 4. Scheme of the XYZ mesh of measurement points travelled by the submerged antenna particularized for the IB2IB scenario.

In case of the IB2OB scenario, the large antenna was located over the external container's wall. In this scenario, two different setups were considered:

- Setup IB2OB.1: The on-body antenna (large antenna) was fixed in the center of the external container's wall whereas the in-body antenna (miniaturized antenna) was located in a XYZ mesh of $19 \times 19 \times 3$ measurement points (see Fig. 4).
- Setup IB2OB.2: The on-body antenna was located in an initial position (in orange color in Fig. 5) and moved away λ , 2λ , 4λ and 8λ in the Y axis, where λ is the wavelength corresponding to the central frequency of the frequency band under analysis considering the propagation speed inside the phantom.

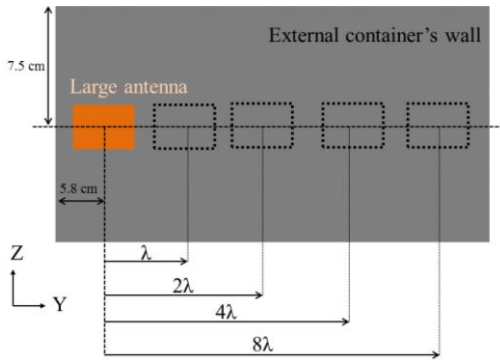


Fig. 5. The locations of on-body antenna in the experimental IB2OB.2 setup.

E. Data Processing

From the measurements, the path loss of each scenario was calculated. It should be highlighted that non-direct paths and wall reflections were highly attenuated due to the lossy propagation medium. Besides, only those S_{21} samples 10 dB above the noise level were taken into account. As a consequence, the received power can be considered to be practically the direct path contribution. The path loss was computed as follows:

$$PL(dB) = -10 \log_{10} \left(\text{mean}(|H(f)|^2) \right), \quad (2)$$

with $H(f)$ being the frequency transfer function in N resolution points computed as $H(f) = |S_{21}| e^{-j\angle S_{21}}$, where $|S_{21}|$ and $\angle S_{21}$ are module and phase in radians of the S_{21} , respectively.

The correlation coefficient between two different channel impulse responses, $h_{d_1}(\tau)$ and $h_{d_2}(\tau)$, was obtained as the maximum of the correlation as follows:

$$\rho_{d_1, d_2}(\tau) = \frac{E[h_{d_1}(\tau) \cdot h_{d_2}^*(\tau)]}{\sqrt{E[|h_{d_1}(\tau)|^2] \cdot E[|h_{d_2}(\tau)|^2]}}, \quad (3)$$

where $E[\]$ is the expectation operation value and $h_{d_i}(\tau)$ is the impulse channel response for a distance between antennas d_i , obtained from the IFFT of the $H(f)$ within N points.

III. PATH LOSS RESULTS

In this section, the path loss models as a function of distance between antennas for both experimental setups are presented.

A. IB2IB scenario

In Fig. 6, the path loss obtained from the measurements for the IB2IB scenario is shown. From this figure, one can observe that the best fit is achieved with a linear approximation model as:

$$PL(dB) = PL_0 + \alpha \cdot d(cm) + X_{\sigma_{IB2IB}}, \quad (4)$$

where PL_0 is the value of the path loss when the distance between antenna centers, d , tends to 0; α is a fitting parameter and $X_{\sigma_{IB2IB}}$ is the shadowing term for IB2IB scenario. In this case, PL_0 (dB) = 45.03 dB and $\alpha = 4.57$ dB/cm. Fig. 7 shows the cumulative distribution function (CDF) of the measurements. It can be noted that the empirical model of shadowing can be fitted by means of a normal distribution with zero mean and standard deviation $\sigma = 4.26$ ($N(0, \sigma)$). It is important to note that the path loss is given from $d = 3$ cm to $d = 8$ cm because most of the measurements above 8 cm were at noise level.

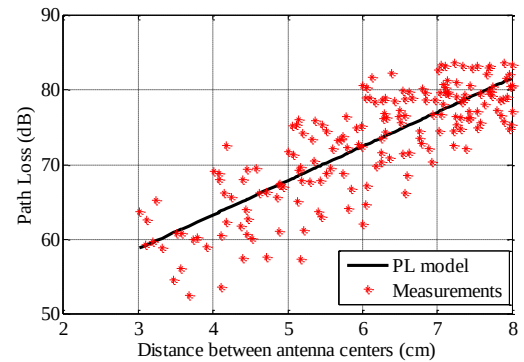


Fig. 6. Path loss as a function of distance between antenna centers (d) in the experimental IB2IB scenario.

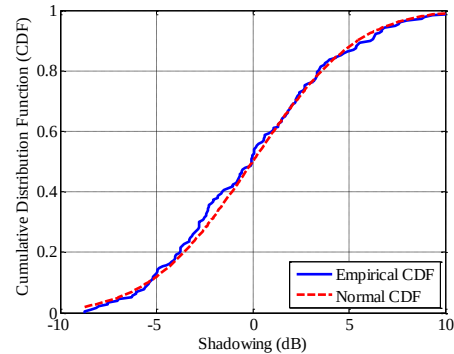


Fig. 7. Shadowing in the experimental IB2IB scenario.

As evidenced by our results, the path loss model has been well-fitted by a linear approximation model. These results are in agreement with other research works which were carried out in other frequency bands [5]. However, the set of measurements presented in this work and those performed in [5] have been performed within different frequency bands and bandwidths. Indeed, there is a lack of measurements for IB2IB configurations within UWB frequency band in the literature.

B. IB2OB scenario

The path loss values obtained for the IB2OB case are shown in Fig. 8. In this case, the path loss was fitted by means of a log-distance model since the measurement points follow this trending within the measured distances. The log-distance equation is given by the following expression:

$$PL(\text{dB}) = PL_{0,d_{ref}} + 10\gamma \log_{10} \left(\frac{d}{d_{ref}} \right) + X_{\sigma_{IB2OB}}, \quad (5)$$

being $PL_{0,d_{ref}}$ the path loss value in a reference distance d_{ref} equal to 1 cm, γ the path loss exponent, d the distance between antenna centers, and $X_{\sigma_{IB2OB}}$ the shadowing term for the IB2OB scenario. In this case, the parameters of the log-distance equation were $PL_{0,d_{ref}} = 47.84$ dB and $\gamma = 1.98$. From Fig. 9, one can also observe that the shadowing also follows a normal distribution with zero mean and $\sigma = 1.2$.

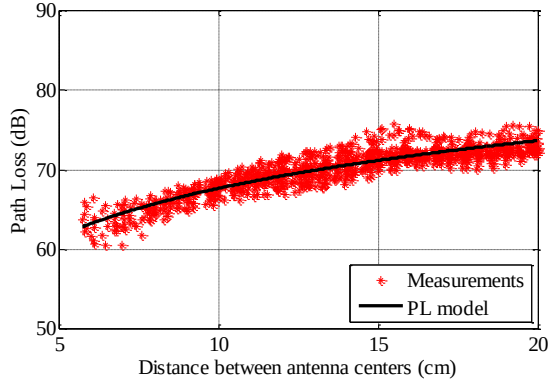


Fig. 8. Path loss as a function of distance between antenna centers (d) in the experimental IB2OB scenario.

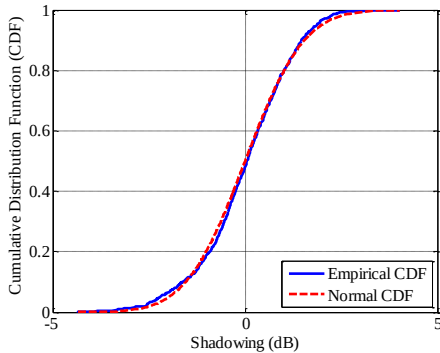


Fig. 9. Shadowing in the experimental IB2OB scenario.

As mentioned above, the path loss model obtained from our measurements follows a logarithmic trend as the distance between antennas increases. In [6], the authors proposed a path loss model from 0 to 12 cm within 1 to 6 GHz in a heterogeneous medium by means of a software simulation. As

it can be checked, our path loss model is similar to that obtained in [6] within the same distance range. However, our IB2OB path loss model is given for a higher range of distances. Moreover, their path loss model is defined within a lower frequency band (1-6 GHz). Besides, our path loss model can also be compared with that obtained from in-vivo measurements [22]. Although our path loss model is defined in distance above 12 cm, the trending of our path loss model and the path loss aforementioned is comparable considering the same range of values for the distance between antennas. However, absolute values of the path loss are different due to the different antennas used in both experiments.

In [10], the authors compared phantom-based and in-vivo measurements in an IB2OB scenario using the phantom described in [14]. As can be seen, the propagation losses in [10] are higher than those obtained using the new phantom. That is by the fact that the dielectric values of the new phantom are close to those obtained by Gabriel in [8]. On the contrary, the phantom proposed in [14] overestimates the losses as concluded in [10].

IV. CORRELATION COEFFICIENTS

The diversity of the channel in transmission and reception is assessed throughout this section. For this purpose, the correlation coefficients in each scenario are computed.

A. IB2IB

For IB2IB scenario, the correlation in transmission for transmitters located in the same XY plane is shown in Fig. 10. In this case, the position of the reference impulse channel response was located at the center of the XY plane at $z = 0$. The distance between antenna centers at this reference location – denoted by subscript d_1 in (2) – was $d_1 = 5.77$ cm. From Fig. 10, it can be deduced that the correlation decreases rapidly as the distance increases in both X and Y axes. Moreover, one can observe that the correlation drops below 0.3, when the transmitting antenna location is more than 1 cm away from the location of the reference transmitter. It should be mentioned that the resolution distance between the measured transmitter positions is 1 cm.

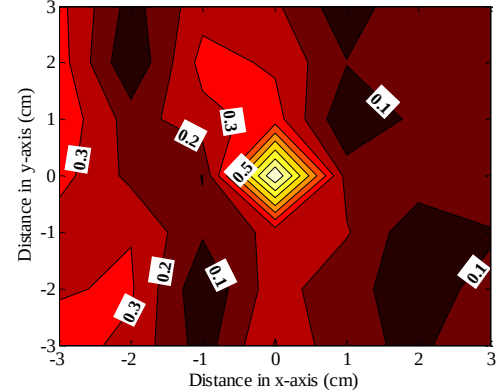


Fig. 10. Correlation coefficients at $z = 0$ in experimental IB2IB scenario.

Fig. 11 shows the correlation in transmission for transmitters located at different XY planes. The reference channel impulse response was correlated with those located in an upper plane. This upper plane was separated at a distance Δz (1 cm). It can be noted that the correlation is lower than 0.3 for all the positions in the upper plane. Hence, it can be

concluded that the channel is highly uncorrelated at different antenna heights.

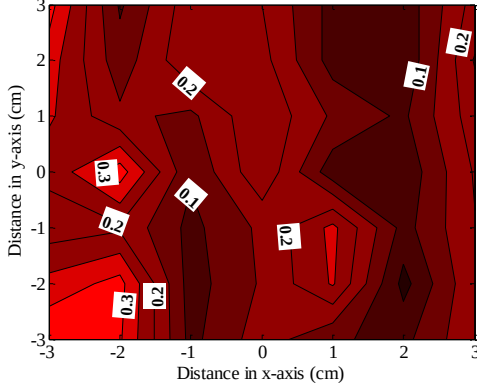


Fig. 11. Correlation coefficients at a distance of Δz from $z = 0$ in experimental IB2IB scenario.

B. IB2OB

In the IB2OB scenario, the correlation in transmission was calculated in the same manner as in the previous case, considering the setup IB2OB.1. Thus, the reference position was located again at the center of the XY plane at $z = 0$, being the distance between antenna centers in this case of $d_1 = 14.83$ cm. Thus, the values of the correlation coefficients are shown in Fig. 12. As can be observed, the correlation in the same XY plane is high in those positions close to the reference one. Thus, the IB2OB channel can be considered to be uncorrelated for transmitting positions separated approximately more than 5 cm in each axis.


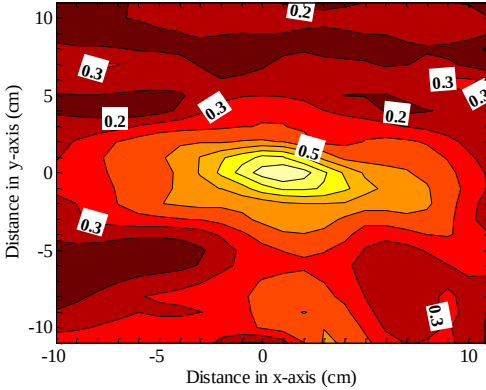


Fig. 12. Correlation coefficients at $z = 0$ in experimental IB2OB.1 scenario.


Fig. 13 shows the correlation in transmission when the position between transmitters was Δz (1 cm) and $2\Delta z$ (2 cm) from the reference position in the Z axis. It can be noted that the correlation is lower as the distance between planes in Z axis increases. This effect can be observed from Fig. 13(a) and Fig. 13(b). On the one hand, in Fig. 13(a) the correlation was reduced with respect to the case of $z = 0$ for all positions. On the other hand, in Fig. 13(b) where the separation distance in Z axis was $2\Delta z$, uncorrelated signals were found whatever the separation of transmitting positions.

In order to evaluate the correlation in reception, the setup IB2OB.2 was considered (see section II.D). Table I shows the correlation coefficients for different receiving antenna positions (see Fig. 5) as a function of different transmitting antenna locations along the X axis. It should be mentioned that for location 0 the transmitting antenna was located again at the

center position of the XY plane. The rest of locations corresponds to Δx steps from location 0 of the transmitter. From table I, one can deduce that the correlation coefficients are lower as the distance between receiving antennas is higher. Besides, the correlation is below 0.5 for a separation distance between receivers above λ . It can be noted that the correlation decreases rapidly as the distance between receivers increases as concluded in [24].

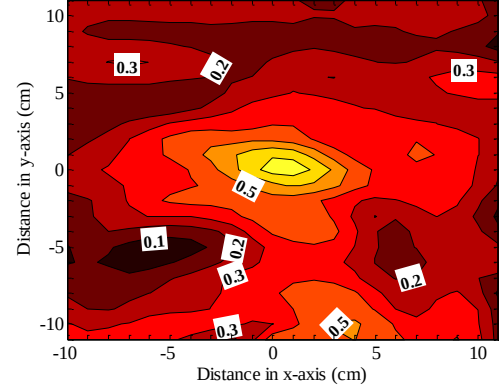

(a)

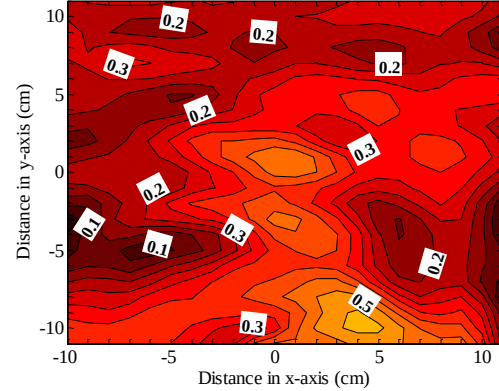

(b)

Fig. 13. Correlation coefficients at a distance of (a) $z = \Delta z$ and (b) $z = 2\Delta z$ from the plane $z = 0$ in experimental IB2OB.1 scenario.

Likewise, Table II shows the correlation coefficients between receiving antennas when the position of the transmitting antenna was varied in the Y axis. In this case, the correlation also decreases when the distance between receiving antennas increases. As in the previous case, the correlation is below 0.5 for distance above λ whatever the position of the transmitting antenna in the Y axis.

TABLE I
CORRELATION COEFFICIENTS ALONG THE X AXIS IN IB2OB.2 SCENARIO

	λ	2λ	4λ	8λ
$-5\Delta x$	0.62	0.37	0.35	0.29
$-4\Delta x$	0.55	0.36	0.28	0.26
$-3\Delta x$	0.54	0.35	0.25	0.25
$-2\Delta x$	0.57	0.36	0.26	0.28
$-\Delta x$	0.63	0.42	0.29	0.24
0	0.65	0.46	0.27	0.18
Δx	0.66	0.46	0.22	0.17
$2\Delta x$	0.67	0.44	0.19	0.18
$3\Delta x$	0.69	0.45	0.20	0.16
$4\Delta x$	0.71	0.47	0.23	0.14
$5\Delta x$	0.73	0.49	0.22	0.14

TABLE II

CORRELATION COEFFICIENTS ALONG THE Y AXIS IN IB2OB.2 SCENARIO

	λ	2λ	4λ	8λ
-5 Δy	0.67	0.46	0.22	0.18
-4 Δy	0.68	0.48	0.24	0.17
-3 Δy	0.66	0.48	0.21	0.17
-2 Δy	0.58	0.42	0.21	0.19
- Δy	0.54	0.35	0.20	0.18
0	0.53	0.37	0.24	0.11
Δy	0.54	0.41	0.32	0.10
2 Δy	0.53	0.39	0.34	0.08
3 Δy	0.50	0.42	0.31	0.17
4 Δy	0.47	0.41	0.32	0.10
5 Δy	0.44	0.37	0.29	0.09

V. CONCLUSIONS

In this paper a set of phantom-based measurements within 3.1-8.5 GHz is presented. As a novelty, a new UWB phantom which mimics the permittivity values of human muscle tissue in the whole UWB frequency band with high accuracy was used. Using this new phantom, in-body to in-body (IB2IB) and in-body to on-body (IB2OB) scenarios were considered. In order to perform the measurements, an automatic 3-axis positioner was used. Thus, a large amount of measurements with high location accuracy were obtained in order to characterize the UWB in-body channel. Two path loss models for IB2IB and IB2OB scenarios were obtained. In the IB2IB case, the path loss model which best fitted the measurements for distances between antennas ranging from 3 to 8 cm was a linear model. In contrast, the path loss was fitted by a log-distance model from 5.5 to 20 cm for the IB2OB scenario.

The diversity of the UWB in-body channel was also investigated by means of the calculation of the correlation coefficients for both scenarios. In the IB2IB case, the correlation in transmission was below 0.5 regardless the distance to the reference transmitter. For the IB2OB scenario, our findings revealed that the use of two receiving antennas separated more than λ is essential to obtain uncorrelated channel impulse responses in reception. Regarding the correlation coefficients between transmitting antennas, it is lower when the transmitters are located in different Z planes for the same XY position. For future works, it would be crucial to manufacture other human phantoms such as fat, skin and so on. In this manner, the effects of the heterogeneity of the human tissues on UWB channel characterization will be checked. These results could be contrasted with simulations by using human voxel models.

REFERENCES

- [1] G. Iddan, G. Meron, A. Glukhovsky, and P. Swain, "Wireless capsule endoscopy," *Nature*, vol. 405, no. 6785, p. 417, May 2000.
- [2] H. Burri and D. Senouf, "Remote monitoring and follow-up of pacemakers and implantable cardioverter defibrillators," *Europace*, vol. 11, no. 6, pp. 701–9, Jun. 2009.
- [3] "IEEE Standard for Local and metropolitan area networks - Part 15.6: Wireless Body Area Networks" pp. 1–271, 2012.
- [4] W. G. Scanlon, J. B. Burns, and N. E. Evans, "Radiowave propagation from a tissue-implanted source at 418 MHz and 916.5 MHz," *IEEE Trans. Biomed. Eng.*, vol. 47, no. 4, pp. 527–34, Apr. 2000.
- [5] R. Chavez-Santiago, C. Garcia-Pardo, A. Fornes-Leal, A. Valles-Lluch, G. Vermeeren, W. Joseph, *et al.*, "Experimental Path Loss Models for In-Body Communications within 2.36-2.5 GHz," *IEEE J. Biomed. Heal. Informatics*, vol. 19, no. 3, pp. 930–937, Apr. 2015.
- [6] R. Chavez-Santiago, K. Sayrafian-Pour, A. Khaleghi, K. Takizawa, J. Wang, I. Balasingham, *et al.*, "Propagation models for IEEE 802.15.6 standardization of implant communication in body area networks," *IEEE Commun. Mag.*, vol. 51, no. 8, pp. 80–87, Aug. 2013.
- [7] X. Shen, M. Guizani, R. Caiming Qiu, and T. Le-Ngoc, Eds., *Ultra-Wideband Wireless Communications and Networks*. John Wiley & Sons, 2007.
- [8] C. Gabriel, "Compilation of the Dielectric Properties of Body Tissues at RF and Microwave Frequencies," Brooks Air Force, N.A./OE-TR-1996-0037, San Antonio, TX, 1996.
- [9] P. A. Floor, R. Chavez-Santiago, S. Brovoll, Ø. Aardal, J. Bergsland, O.-J. H. N. Grymyr, *et al.*, "In-Body to On-Body Ultra Wideband Propagation Model Derived from Measurements in Living Animals," *IEEE J. Biomed. Heal. Informatics*, vol. 19, no. 3, pp. 1–1, 2015.
- [10] C. Garcia-Pardo, R. Chavez-Santiago, N. Cardona, and I. Balasingham, "Experimental UWB frequency analysis for implant communications," in *37th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBC)*, Milan, 2015, pp. 5457–5460.
- [11] H. Xie, V. Shamdassani, A. T. Fernandez, R. Peterson, M. Lachman, Y. Shi, *et al.*, "Shear wave Dispersion Ultrasound Vibrometry (SDUV) on an ultrasound system: In vivo measurement of liver viscoelasticity in healthy animals," in *IEEE International Ultrasonics Symposium*, 2010, pp. 912–915.
- [12] A. Khaleghi, R. Chávez-Santiago, and I. Balasingham, "Ultra-wideband statistical propagation channel model for implant sensors in the human chest," *IET Microwaves, Antennas & Propag.*, vol. 5, no. 15, p. 1805, 2011.
- [13] R. Chavez-Santiago, C. Garcia-Pardo, A. Fornes-Leal, A. Valles-Lluch, I. Balasingham, and N. Cardona, "Ultra wideband propagation for future in-body sensor networks," in *IEEE 25th Annual International Symposium on Personal, Indoor, and Mobile Radio Communication (PIMRC)*, 2014, pp. 2160–2163.
- [14] H. Yamamoto, J. Zhou, and T. Kobayashi, "Ultra Wideband Electromagnetic Phantoms for Antennas and Propagation Studies," *IEICE Transactions on Fundamentals of Electronics, Communications and Computer Sciences*, vol. E91-A, no. 11, pp. 3173–3182, Nov. 2008.
- [15] M. Lazebnik, E. L. Madsen, G. R. Frank, and S. C. Hagness, "Tissue-mimicking phantom materials for narrowband and ultrawideband microwave applications," *Phys. Med. Biol.*, vol. 50, no. 18, pp. 4245–58, Sep. 2005.
- [16] T. Yilmaz, R. Foster, and Y. Hao, "Broadband Tissue Mimicking Phantoms and a Patch Resonator for Evaluating Noninvasive Monitoring of Blood Glucose Levels," *IEEE Trans. Antennas Propag.*, vol. 62, no. 6, pp. 3064–3075, Jun. 2014.
- [17] S. Gezici, G. B. Giannakis, H. Kobayashi, A. F. Molisch, H. V. Poor, and Z. Sahinoglu, "Localization via ultra-wideband radios: a look at positioning aspects for future sensor networks," *IEEE Signal Process. Mag.*, vol. 22, no. 4, pp. 70–84, Jul. 2005.
- [18] B. Moussakhani, J. T. Flåm, S. Støa, I. Balasingham, and T. Ramstad, "On localisation accuracy inside the human abdomen region," *IET Wirel. Sens. Syst.*, vol. 2, no. 1, p. 9, 2012.
- [19] M. Marinova, A. Thielens, E. Tanghe, L. Vallozzi, G. Vermeeren, W. Joseph, *et al.*, "Diversity Performance of Off-Body MB-OFDM UWB-MIMO," *IEEE Trans. Antennas Propag.*, vol. 63, no. 7, pp. 3187–3197, Jul. 2015.
- [20] N. Cardona, S. Castelló-Palacios, A. Fornes-Leal, C. Garcia-Pardo, and A. Vallés-Lluch, "Modelo sintético de tejidos biológicos para la evaluación de la transmisión inalámbrica de ondas electromagnéticas," ES Patent 2 575 731, Dec. 22, 2015. [in Spanish]
- [21] C. Tarin, P. Marti, L. Traver, N. Cardona, J. A. Diaz, and E. Antonino, "UWB Channel Measurements for Hand-Portable Devices: A Comparative Study," in *IEEE 18th International Symposium on Personal, Indoor and Mobile Radio Communications*, 2007, pp. 1–5.
- [22] C. Garcia-Pardo, N. Cardona, A. Fornes-Leal, I. Balasingham, R. Palomar, J. Bergsland, *et al.*, "Experimental Ultra Wideband Path Loss Models for Implant Communications," in *27th IEEE International Symposium on Personal, Indoor and Mobile Radio Communications*, Valencia, Sept. 4-7, 2016.
- [23] R. K. Makoto Kawasaki, "A TOA Based Positioning Technique of Medical Implanted Devices," *3rd International Symposium on Medical Information & communication Technology (ISMICT)*, 2008, Montreal, Canada.
- [24] J. Shi, S. Member, D. Anzai, and J. Wang, "Channel Modeling and Performance Analysis of Diversity Reception for Implant UWB Wireless Link," *IEICE Trans. Commun.*, vol. E95.B, no. 10, p. 3197–205, 2012.



Carlos Andreu was born in Valencia, Spain. He received the M.Sc. degree in telecommunication engineering from the ETSI Telecommunications at the Universitat Politècnica de València, Valencia, Spain, in 2013.

Since November 2014, he is with the Institute of Telecommunications and Multimedia Applications (iTEAM) as a Ph.D. candidate. His research work is focused on the in-body channel characterization within high frequency bands, as well as on the design of tiny implantable antennas for enhancing the current wireless healthcare systems.



Sergio Castelló-Palacios was born in Valencia, Spain. He received the M.Sc. degree in chemical engineering from the School of Industrial Engineering at the Universitat Politècnica de València, Valencia, Spain, in 2015.

He is with the Centre for Biomaterials and Tissue Engineering since September 2014. At the moment, he is pursuing a Ph.D. degree. He is focused on developing tissue-equivalent materials in order to test microwave technologies, mainly antennas that will be used for transmitting in wireless body area networks.



Concepcion Garcia-Pardo attended the Universidad Politécnica de Cartagena, Cartagena, Spain, where she graduated in telecommunication engineering in 2007 and she received the M.Sc. degree in information technologies and communications in 2008.

In 2012 she received her Ph.D. degree from the Universidad Politécnica de Cartagena, and Ph.D. degree in Microwaves and Microtechnologies from the Lille 1 University. Her Ph.D. Thesis was awarded the special prize from the Universidad Politécnica de Cartagena in 2013. In 2011 and 2012 she was a lecturer at the Universidad Politécnica de Cartagena, in the area of Signal Theory and Communications. In 2012 she joined the Institute of Telecommunications and Multimedia Applications (iTEAM) as a postdoc researcher. Her current work is focused on implant communications for body area networks.



Alejandro Fornes-Leal was born in Denia, Spain. He received the M.Sc. degree in telecommunication engineering from the ETSI Telecommunications at the Universitat Politècnica de València, Valencia, Spain, in 2014.

Since February 2014, he is with the Institute of Telecommunications and Multimedia Applications (iTEAM), Valencia, as a Researcher. Recently, he is working towards a Ph.D. degree. His current work is mainly focused on the electromagnetic characterization of materials and human tissues, as well as on the development of medical applications that aid in the diagnosis of colorectal cancer.



Ana Vallés-Lluch received the M.Sc. degree in chemical engineering and the Ph.D. degree from the Universitat Politècnica de València, Valencia, Spain, in 2001 and 2008, respectively.

She is currently an Associate Professor of Biomaterials and Thermodynamics at the School of Industrial Engineering at the Universitat Politècnica de València and member of the Centre for Biomaterials and Tissue Engineering and of the Department of Applied Thermodynamics. Her research interests include biomaterials and tissue engineering, in particular in the development of materials with controlled chemistry and microporous structures tailored for the intended application, their morphological, physicochemical, and mechanical characterization and of their interaction with the biological environment.



Narcís Cardona was born in Barcelona, Spain. He received the M.S. degree in communications engineering from the ETSI Telecommunications at the Universitat Politècnica de Catalunya, Barcelona, Spain, in 1990, and the Ph.D. degree in telecommunications from the Universitat Politècnica de València, Valencia, Spain, in 1995.

Since October 1990, he is with the Communications Department of the Universitat Politècnica de València where he heads the Mobile Communications Group. He is also the Vice-Director of the Research Institute of Telecommunications and Multimedia Applications (iTEAM) since 2004. Prof Cardona has led and participated in National and European research projects, Networks of Excellence and other research forums. At the European scale, he has been Vice-Chairman of COST Action IC273, Chair of the WG3 of COST Action IC2100 in the area of Radio Access Networks, and Chairman of the COST Action IC1004. He is also a member of the Steering Board, METIS (7FP), and in Future Mobile Communications Technologies. His current areas of interest include mobile channel characterization, broadcast cellular hybrid networks and body area networks.